


## ARTWORK PREPARATION FOR AN ARCH STAND 900

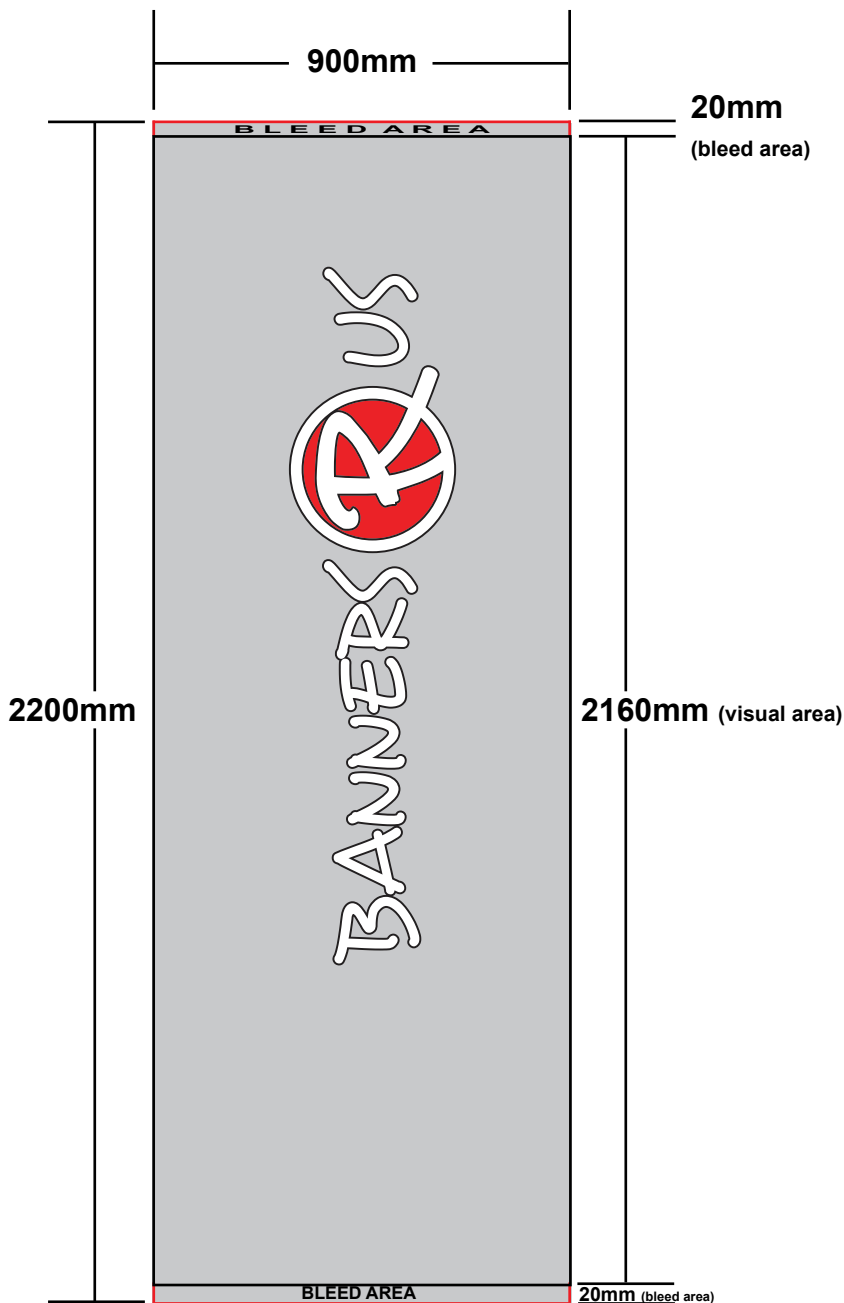

### Arch Stand 900

#### Visual area: 900(w) x 2160(h)

Ensure that all text and logos are kept within this area. PLEASE NOTE this is not a retractable stand and requires manual set up.

#### Bleed area(s):

These areas are required for attachment to the system, they are inserted into the frame, and are not visible when erect.

For a clean finish on your display make sure any background colours or graphics bleed off into these areas.

#### Setup:

Make sure all images are at least 300dpi at final size, if you are unable to source high resolution images it is recommended to request an at-size proof of a portion of your banner to check quality.

#### Acceptable file types

High Resolution PDF, Corel Draw 11, Adobe Illustrator, Photoshop TIFF, JPG (300dpi), EPS (Encapsulated Postscript). If your file contains type, make sure you send a copy all fonts used or convert all type to curves. (We cannot use Mac fonts so please convert these to outlines (curves))

If you have any further queries please don't hesitate to call us on **1800 995 399**

**email [info@bannersrus.com.au](mailto:info@bannersrus.com.au)**

**[www.bannersrus.com.au](http://www.bannersrus.com.au)**